

Effect of dose rate on antitumor activity in hypoxic cells by using flattening filter free beams

T. Hara^{1, 2}, M. Tominaga^{3*}, K. Yajyu¹, R. Kouzaki¹, A. Hanyu¹, H. Yamada⁴, M. Sasaki⁵, S. Azane⁵, Y. Uto^{4*}

¹Graduate School of Technology and Science, Tokushima University, Tokushima, Japan

²Marketing Department, Varian Medical Systems K.K., Tokyo, Japan

³Institute of Health Science, Tokushima University, Tokushima, Japan

⁴Institute of Bioscience and Bioindustry, Tokushima University, Tokushima, Japan

⁵Radiological Technology, Tokushima University Hospital, Tokushima, Japan

ABSTRACT

Background: Recently, the Flattening Filter Free (FFF) beams, which allow a dose rate increase of up to four times compared to the normal dose rate, have been incorporated into radiation therapy machines. The aim of this study is to evaluate antitumor activity in hypoxic cells irradiated with different dose rates using FFF beams and to identify the casual mechanism for cellular damage during irradiation.

Materials and Methods: EMT6 cells were treated with 95% N₂ and 5% CO₂ to maintain a hypoxic condition. Three dose rates, namely, 6.27 Gy/min, 12.00 Gy/min, and 18.82 Gy/min, were used to deliver the prescribed dose of 2 to 4 Gy using the TrueBeam linear accelerator. The number of colonies was counted to evaluate the cell surviving fraction. To investigate the mode of action, additional experiments to detect reactive oxygen species (ROS) by aminophenyl fluorescein (APF) assay, and DNA double-strand breaks (DSBs) by γH2AX assay were performed. **Results:** Irradiation of hypoxic cells using FFF beams increases antitumor activity as a function of dose rate. The fluorescence of the APF assay was significantly increased when high dose rates were used. In addition, results from our γH2AX assays show that the number of DNA DSBs increased as a function of dose rate, in hypoxic cells. **Conclusion:** We demonstrate that there is a significant dose rate-dependent difference in antitumor activity in hypoxic cells, when FFF beams are used.

Keywords: Flattening filter free (FFF), radiation biology, hypoxic cell, dose rate effect.

► Original article

*Corresponding authors:

Dr. M. Tominaga, Dr. Y. Uto,

Fax: +81 886567514

E-mail:

uto.yoshihiro@tokushima-u.ac.jp

Revised: July 2017

Accepted: August 2017

Int. J. Radiat. Res., April 2018;
16(2): 197-205

DOI: 10.18869/acadpub.ijrr.16.2.197

INTRODUCTION

Stereotactic body radiotherapy (SBRT) is one of the favoured methods used in radiation therapy for the treatment of cancers affecting the thoracic region. SBRT uses large doses of radiation per fractionation of treatment, and as a result, the treatment procedure is completed in only a few fractions. However, using large doses also results in increased treatment time; thereby, limiting the determination of a patient's status. Furthermore, the intrafractional motion

may also limit the dose reaching the target during the procedure ⁽¹⁾. SBRT is mainly employed in the treatment of cancers affecting the abdominal or thoracic region where respiratory movement occurs during treatment. Technologies have been developed to account for the respiratory movement in order to minimize normal tissue complications from internal organ displacement ⁽²⁾. To achieve the best dose coverage to the tumor without expanding margins, the option of using respiratory-gated treatment is also available ⁽³⁾.

During the respiratory-gated treatment procedure, beams terminate automatically when the patient's respiratory motion deviates from a predefined gated area. This procedure therefore requires longer treatment times, the shortening of which is highly desirable.

Recently, the FFF beams, which allow for the dose rate to be increased by up to four times compared to the normal dose rate, have been incorporated into many radiation therapy machines ⁽⁴⁻⁸⁾. The most beneficial aspect of using FFF beams is the shortening of treatment time, thereby improving patient's comfort and total throughput. Prendergast *et al.* ⁽⁹⁾ reported that the use of FFF beams enabled the reduction of the average treatment time for an SBRT patient from 46 to 26 min. A further advantage of using the FFF beams is reduction of the outside field dose to the patient due to removal of the flattening filter, which provides a scattered radiation dose into the patient ⁽¹⁰⁾. These advantages have led clinicians to initiate the clinical use of FFF beams ⁽¹¹⁻¹⁶⁾. However, questions remain concerning the effects of irradiating patients with significantly larger doses in short time periods.

Wang *et al.* ⁽¹⁷⁾ observed surface dose increases during treatments using FFF beams. Mu *et al.* ⁽¹⁸⁾ and Moiseenko *et al.* ⁽¹⁹⁾ also reported that the cell survival rate was higher when the total time for irradiating the cell was longer, indicating that irradiation time may have an effect on cell survival. Studies conducted by Lohse *et al.* ⁽²⁰⁾ reported the effect of high dose per pulse on cancer cell survival, comparing 10 MV X-rays with flattening filter (10 X) and FFF (10 X FFF) by using the dose of 5 Gy or 10 Gy. They concluded that the higher the dose rate, the lower the cell survival rates, especially for irradiation of 10 Gy. They also demonstrated that there is no significant difference in cell survival rates when irradiation was carried out using 10 X and 10 X FFF beams at the prescribed dose of 5 Gy. However, when using irradiation of 10 Gy and above, the cell survival rate decreased as the prescribed dose increased. These findings are in contrast to recent reports from Karan *et al.* ⁽²¹⁾ who showed that there is no significant difference in cell survival rate when the same

energy was used with or without the flattening filter at the same prescribed dose. Therefore, it remains unclear as to whether the usage of high dose rate using FFF beams affects cell survival rate.

The main cause of radiation damage to the cell can be due either to direct or indirect action of radiation on DNA. It is known that about two-thirds of the damage inflicted on DNA by low-linear energy transfer (LET) ionization occurs indirectly ⁽²²⁾. During indirect action, radiation hits water molecules leading to the production of ROS. DSBs in DNA, by the direct or indirect action of radiation, are also very common triggers of cell damage. Nunez *et al.* ⁽²³⁾ reported a linear relationship between DSBs and irradiation dose. It is the general consensus that the solid tumor cells are under hypoxic conditions; for low -LET radiation, the radiation dose required to achieve the same biological effect is up to three times higher in hypoxic cells than in cells with normal oxygen levels ⁽²⁴⁻²⁵⁾. Under hypoxic conditions, DNA is oxidized by ROS, but simultaneously it is neutralized by accepting an electron from hydrated electron. However, hydrated electron reacts with oxygen when present, thus no overall neutralization of ROS is observed and DNA damage occurs ⁽²⁶⁾. As mentioned previously, studies investigating the effect of dose rates employing FFF beams are limited. Furthermore, these reports do not consider the cell oxygenation status. Studies focusing on the use of FFF beams for treatment of hypoxic cancer cells are yet to be conducted. We suggest that the cell oxygenation conditions should be considered in experiments aimed at studying the effect of dose rate, when using FFF beams, due to the hypoxic nature of many tumors. Clearly demonstrating the effect of FFF on hypoxic cancer cells would provide invaluable information to the radiation oncologist. The purpose of the present study is to evaluate the effect of dose rate when using FFF beams on cells with a different oxygenation status, while considering antitumor activity. Additionally, we also carried out APF and γ H2AX assays to determine the mechanisms of cell damage.

MATERIALS AND METHODS

Cell cultures

EMT6 mouse mammary tumor cell line, a widely used model in radiation biology, was obtained from Kyoto University (Kyoto, Japan). The cells were cultured in Eagle's MEM medium (Sigma-Aldrich Japan, Tokyo, Japan) supplemented with 10 % fetal bovine serum (JR Scientific Inc., Woodland, CA, USA). The cells were incubated at 37°C, with 5% CO₂ in a subconfluent state. Aliquots were collected from the suspension medium containing 4×10⁴ cells/mL, and 500 µL of the cell suspension was dispensed into test tubes. This was then treated with 95% N₂ and 5% CO₂ for 15 min to simulate hypoxic conditions. We confirmed that the tumor cells were under a sufficient hypoxic state by calculating the oxygen enhancement ratio (OER). OER was calculated by dividing the irradiation dose for hypoxic cells by the irradiation dose for aerobic cells required to give a surviving fraction of 10 %. The observed OER under hypoxia after 15 min of exposure to N₂ was 3.12.

Irradiation

The TrueBeam linear accelerator (Varian Medical Systems, Palo Alto, CA, USA) was used for irradiation. The cell lines were irradiated to the prescribed doses of 2 Gy and 4 Gy with nominal energy of 10 X without flattening filter (10 X FFF). Different dose rates (6.27 Gy/min, 12.00 Gy/min, and 18.82 Gy/min) were selected to irradiate the absorbed dose. Following irradiation, the test tubes were centrifuged at 1,500 rpm for 10 min to fix the cells. The cells were re-suspended and 500 cells were placed in three dishes for each experiment. All dishes were then incubated at 37°C for 7 days to allow colonies to form. After incubation, cells were washed to remove any leftover media, and fixed on the dishes by adding 2 mL of methanol for 10 min. Following the removal of methanol, 2 mL of 5% Giemsa stain was added and the colonies were stained for 60 min. The number of colonies was counted manually.

Reactive oxygen species detection by aminophenyl fluorescein assay

To support the results from the colony formation assay, an APF assay (Sekisui Medical Co. Ltd., Tokyo, Japan) was performed. A 5 mM solution of APF was diluted with 100 mM sodium phosphate buffer to attain a concentration of 100 µM and dispensed into test tubes, each containing 500 µL. After irradiating of 2 Gy at different dose rates (6.27 Gy/min, 12.00 Gy/min, and 18.82 Gy/min), the cells were placed into a multi-well black plate (100 µL per well). Fluorescence was measured using excitation and emission wavelengths of 490 nm and 515 nm, respectively. Non-irradiated cells were prepared as the control group.

DNA double strand breaks detection by γH2AX assay

We used the γH2AX assay to support data from the experiments described above. One day prior to treatment, cells from the EMT6 cell line were placed onto a slide chamber at a concentration of 2×10⁴ cells/mL. Following irradiation, cells were fixed in 4% paraformaldehyde (Wako Pure Chemical Industries, Ltd., Tokyo, Japan) for 10 min. Subsequently, fixed cells were permeabilized with 0.5% Triton-X100 (Sigma-Aldrich Japan, Tokyo, Japan) in phosphate-buffered saline (PBS) then blocked with 1.0% bovine serum albumin (BSA) and 0.2% Triton-X100 in PBS. For the γH2AX colocalization experiments, cells were incubated with anti-phospho-histone H2AX (Ser139), antibody clone JBW301 (Merck KGaA, Darmstadt, Germany), and donkey anti mouse IgG antibody-fluorescein isothiocyanate (FITC) conjugate (Merck). Cells were then stained with 4', 6-diamidino-2-phenylindole (DAPI) (Dojindo, Kumamoto, Japan) in PBS for 15 min, and the slides were mounted with Malinol (Muto Pure Chemicals Co. Ltd., Tokyo, Japan). The γH2AX foci were counted manually in the nuclei of 100 cells using a BZ-X700 fluorescence microscope (Keyence, Osaka, Japan) following 2 Gy irradiation; the data shows the average value per cell. We tracked γH2AX foci at 1 h and 24 h of 2 Gy irradiation under

hypoxic and aerobic conditions, to consider the possible involvement of DSB repair.

Statistical validation

The data represents the results of assays performed in triplicate. Data are expressed as mean and standard deviation (SD) values. The statistical significance of the differences between the results of the independent experiments was analysed using the *t*-test of Excel 2010 (Microsoft, Washington, USA). A *p*-value of <0.05 was considered statistically significant.

RESULTS

Cell survival

The average cell surviving fractions (SF), plating efficiency (PE), and SD for dose rates 6.27 Gy/min, 12.00 Gy/min, and 18.82 Gy/min are presented in table 1. The effect of dose rates on cell survival in hypoxic and aerobic cells is plotted in figure 1(a). Using hypoxic cells, we observed that increasing the dose rate, while using FFF beams, showed an increase in antitumor activity in a dose rate-dependent manner. This suggests that a mechanism exists to induce damage in hypoxic cells involving higher dose rates. Conversely, there were no significant dose rate-dependent differences with respect to cell survival in aerobic cells. The comparison of cell survival between hypoxic and aerobic cells is depicted as a histogram in figure 1(b). At the prescribed dose of 4 Gy, resistance to radiation was observed in hypoxic cells.

Aminophenyl fluorescein assay

To further investigate the cause of cell damage, we performed the APF assay to detect formation of ROS. The ratio of fluorescence intensity for the control, and dose rates of 6.27 Gy/min, 12.00 Gy/min, and 18.82 Gy/min are 1.78, 1.88, and 1.94 for hypoxic cells, and 2.01, 2.10, and 2.15 for aerobic cells, respectively (figure 2). The SD value is 0.051, 0.057, and 0.047 for hypoxic cells and 0.029, 0.019, and 0.009 for aerobic cells, respectively.

γ H2AX assay

At the prescribed dose of 2 Gy, the number of DNA DSBs at different dose rates and level of cell oxygenation were determined using the γ H2AX assay at 1 h and 24 h following irradiation (figure 3). There are significant differences in the number of DNA DSBs between irradiated and non-irradiated cells (figure 4). The number of DNA DSBs increased proportionally with the dose rate. By comparing the time course of the number of γ H2AX foci under hypoxic condition, there is no significant difference between 1 h and 24 h following irradiation (figure 4(a)). The SD values for hypoxic cells at zero radiation, and at dose rates of 6.27 Gy/min, 12.00 Gy/min, and 18.82 Gy/min are 0.584, 1.400, 1.546, and 1.728 at 1 h; and 0.486, 1.266, 1.505, and 2.467 at 24 h, respectively. Using aerobic cells, the number of γ H2AX foci significantly decreases after 24 h of irradiation compared to 1 h of irradiation (figure 4(b)). The SD values for aerobic cells at zero radiation and the different dose rates are 0.852, 1.715, 3.696, and 0.949 at 1 h; 0.125, 0.688, 0.643, and 0.725 at 24 h, respectively.



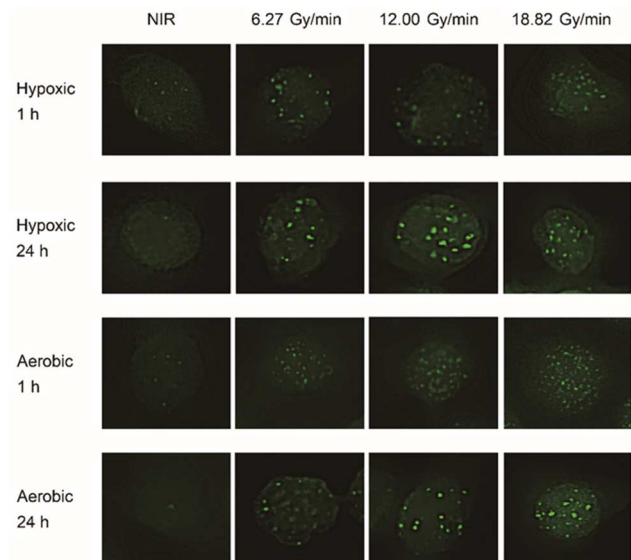



Figure 1. (a) SF of EMT6 cells after irradiation plotted as a function of different dose rates (6.27 Gy/min, 12.00 Gy/min, and 18.82 Gy/min) at 2 and 4 Gy. (b) The differences in SF between hypoxic and aerobic cells as a function of different dose rates at 4 Gy. The error bars represent SD calculated for three independent measurements. **p*<0.05, ***p*<0.01, ****p*<0.005.

Table 1. Surviving fraction and plating efficiency of EMT6 cells after irradiation.

Cell status	Dose (Gy)	Dose Rate (Gy/min)	PE	SF	SD
Hypoxic	0	0.00	0.640	1.000	0.000
		6.27	0.507	0.791	0.049
		12.00	0.450	0.703	0.011
		18.82	0.406	0.635	0.016
	4	6.27	0.358	0.557	0.027
		12.00	0.320	0.497	0.031
		18.82	0.292	0.452	0.038
Aerobic	0	0.00	0.532	1.000	0.000
		6.27	0.378	0.700	0.167
		12.00	0.345	0.649	0.129
		18.82	0.339	0.651	0.159
	4	6.27	0.203	0.393	0.066
		12.00	0.180	0.320	0.091
		18.82	0.165	0.329	0.081

**Figure 2.** Mean ROS values measured using APF fluorescence shown as a function of dose rate in hypoxic and aerobic cells at 1 h following irradiation at 2 Gy. The error bars represent SD calculated for three independent measurements. * $p<0.05$, ** $p<0.01$, *** $p<0.005$ **Figure 3.** Cell lines under hypoxic and aerobic conditions showing γ H2AX foci indicating DNA DSBs with (a) no irradiation (NIR), and 2 Gy irradiation at (b) 6.27 Gy/min, (c) 12.00 Gy/min, and (d) 18.82 Gy/min after 1 h and 24 h of irradiation.**Figure 4.** (a) Overall mean number of γ H2AX foci following 2 Gy irradiation using 6.27 Gy/min, 12.00 Gy/min, and 18.82 Gy/min at 1 h and 24 h for hypoxic cells. (b) Overall mean number of γ H2AX foci following 2 Gy irradiation using 6.27 Gy/min, 12.00 Gy/min, and 18.82 Gy/min at 1 h and 24 h for aerobic cells. The error bars represent SD for three independent measurements. * $p<0.05$

DISCUSSION

In this study, we evaluated the effect of different dose rates on cell survival in aerobic and hypoxic cells by using FFF beams. The effects of dose rates on different cell types have been previously studied by various groups. We suggest that the cell oxygenation condition needs to be considered in experiments aimed at studying the effect of dose rate when using FFF beams. From figure 1(a), it is evident that increasing the dose rate results in increased antitumor activity in hypoxic cells. Therefore, a correlation exists between the dose rate and antitumor activity in a dose rate-dependent manner. The present study was carried out in accordance with the study conducted by Wozny *et al.* ⁽²⁷⁾, who evaluated the effects of dose rate variation on cell survival using a 250-kV irradiator. However, those observations did not correspond to results in a previous report from Karan *et al.* ⁽²¹⁾, where they did not see the dose rate effect on cell survival by using FFF beams. In our study, we did not observe any dose rate effects on cell survival in the cells without hypoxic treatment, which is in agreement with the study reported by Karan *et al.* ⁽²¹⁾. We also compared cell SF between hypoxic and aerobic conditions and demonstrated that the hypoxic cells were more resistant to radiation than aerobic cells. This observation can be explained based on the fact that hypoxic cells showed less DNA damage by radiation. These conclusions are supported by the results of Bristow and Hill ⁽²⁸⁾ and Mathews *et al.* ⁽²⁹⁾. In aerobic cells, the presence of oxygen could aid in the neutralization of hydrated electron, thereby no neutralization of ROS is observed, and as a result DNA is damaged ⁽²⁶⁾. The OER of this study was 3.12 for treatment with N₂ gas for 15 min, which concurs with data by Rockwell and Kallman ⁽³⁰⁾. Our data shows a significant difference between the cell survival of aerobic and hypoxic cells as shown in figure 1(b). The question remains as to why the SF is related in a dose rate-dependent manner only under hypoxic conditions; we therefore performed several assays. As the mechanism of cell damage is mainly due to direct or indirect interaction with ROS, we

investigated ROS production by measuring APF fluorescence using the procedure described by Setsukinai *et al.* ⁽³¹⁾. The data showed that there was a significant difference in fluorescence intensity as a function of dose rate on both hypoxic and aerobic cells. This indicated that ROS production, which could be hydroxyl radical, peroxyxynitrite or hypochlorite, from the interaction of ionizing radiation with water molecules, increases at higher dose rates. In general, the number of ROS produced by ionizing radiation depends on the dose, not the dose rate. Our data clarifies that the use of high dose rate, for short irradiation time, causes more efficient generation of ROS per unit time compared to using lower dose rates. To test the hypothesis that an increase in ROS production will increase DNA damage, we carried out the γ H2AX assay to ascertain whether any DNA DSBs were induced. The data from the γ H2AX assay are presented in figure 4. From the figure, it is clear that there is a significant difference between the numbers of DNA DSBs in cells that are irradiated with different dose rates to those that have undergone zero irradiation, with the number of DNA DSBs increasing as a function of the dose rate on hypoxic cells. This raises another question, as the number of ROS increases proportionally with the dose rate both on aerobic and hypoxic cells, while the cell SF was dose rate-dependent only in hypoxic cells. We hypothesize that this is due to a lack of repair from DNA damage under hypoxic conditions. We considered the possible involvement of DNA DSB repair by acquiring time course data of the number of γ H2AX foci following irradiation. From figure 4(a), it is evident that the number of DSBs does not change significantly 24 h after irradiation under hypoxic conditions. In contrast, from figure 4(b), it is obvious that the number of DSBs significantly decreases after 24 h of irradiation under aerobic conditions. These results support our hypothesis, whereby the aerobic cells are damaged by ROS resulting in DNA DSBs, but some of the damaged DNA may be repaired due to the existing oxygen. For the hypoxic cells however, repair of DNA damage is limited as previously reported in other research ⁽³²⁾. It

clarifies why we could see the dose rate effect for induced ROS with both aerobic and hypoxic cells, but could not see the dose rate effect for cell survival with aerobic cells. This interesting result is also supported by Kumareswaran *et al.*, who observed the decrease of γ H2AX foci after the irradiation only in anoxic human fibroblasts⁽³³⁾. We hypothesize that the temporal DNA damage observed in the control group, is caused by physical damage during the transference of cells between facilities, and not fatal error, since we could observe the cell proliferation after 24 h as seen in figure 5. Moreover, the amount of γ H2AX foci is higher after 1 h compared to 24 h in the control group. It could be explained that the cells at 1 h were at the logarithmic-growth phase, and high cell proliferation triggered the high amount of γ H2AX foci, whereas the cells at 24 h were at the stationary phase, hence cell proliferation is almost stable and so the amount of γ H2AX foci was lower⁽³⁴⁾.

For the hypoxic cells, we suggest that irradiation using high dose rates with FFF beams results in increased production of ROS, which in turn induces a greater number of DNA DSBs without adequate repair of DNA damage. Therefore, we conclude that antitumor activity observed in hypoxic cells is dose rate-dependent.

In our experiments, we pronominally irradiated cells with 2 Gy, which is the prescribed dose in conventional radiation therapy. As mentioned earlier, FFF beams can be used more efficiently in SBRT to reduce the

treatment time, and this is already being implemented in many clinics. Numerous reports regarding FFF beams suggest using a prescribed dose of 8 Gy and above. Kretschmer *et al.*⁽³⁵⁾ reported that FFF beams may be used in conventional radiation therapy and concluded that FFF beams may also be feasible for use in 3D conventional radiation therapy. Zhang *et al.*⁽³⁶⁾ described the use of FFF beams in intensity modulated radiotherapy for upper thoracic carcinoma of the esophagus, which helped in better lung-sparing compared to treatment using flattening filter. Thus, the use of the prescribed dose of 2 Gy in our experiments is appropriate to further investigate the possibility of using FFF beams in conventional radiation therapy.

Our study clearly demonstrates that the antitumor activity in hypoxic cells exhibits significant differences in a dose rate-dependent manner by using FFF beams. We also showed that hypoxic cells were more resistant to radiation compared to aerobic cells by using FFF beams. Increasing the dose rate resulted in the generation of ROS that trigger DNA DSBs, thus, a reduction in cell survival was observed. Based on the findings of our study, we conclude that the usage of a high dose rate in FFF beams may provide superior tumor control in conventional radiotherapy. Further studies are needed to determine the intracellular interactions that govern the observed phenomenon.

Conflicts of interest: Declared none.




Figure 5. Cells proliferation status in the control group at 1h and 24h. Cells were stained with DAPI (4', 6-diamidino-2-phenylindole).

REFERENCES

- Xiao Y, Kry SF, Popple R, et al. (2015) Flattening filter-free accelerators: a report from the AAPM Therapy Emerging Technology Assessment Work Group. *J Appl Clin Med Phys*, **16**(3): 12-29.
- Beddar AS, Kainz K, Briere TM, et al. (2007) Correlation between internal fiducial tumor motion and external marker motion for liver tumors imaged with 4D-CT. *Int J Radiat Oncol Biol Phys*, **67**(2): 630-638.
- Wang PM, Hsu WC, Chung NN, et al. (2014) Feasibility of stereotactic body radiation therapy with volumetric modulated arc therapy and high intensity photon beams for hepatocellular carcinoma patients. *Radiat Oncol*, **9**(18).
- Chang Z, Wu Q, Adamson J, et al. (2012) Commissioning and dosimetric characteristics of TrueBeam system: Composite data of three TrueBeam machines. *Med Phys*, **39**(11): 6981-7018.
- Georg D, Knöös T, McClean B (2011) Current status and future perspective of flattening filter free photon beams. *Med Phys*, **38**(3): 1280-1293.
- Hrbacek J, Lang S, Klöck S (2011) Commissioning of photon beams of a flattening filter-free linear accelerator and the accuracy of beam modeling using an anisotropic analytical algorithm. *Int J Radiat Oncol Biol Phys*, **80**(4): 1228-1237.
- Muralidhar KR, Rout BK, Ramesh KKD, et al. (2015) Small field dosimetry and analysis of flattening filter free beams in true beam system. *J Cancer Res Thera*, **11**(1): 136-140.
- Alongi F, Clerici E, Pentimalli S, et al. (2012) Initial experience of hypofractionated radiation retreatment with true beam and flattening filter free beam in selected case reports of recurrent nasopharyngeal carcinoma. *Rep Pract Oncol Radiother*, **17**: 262-268.
- Prendergast BM, Fiveash JB, Popple RA, et al. (2013) Flattening filter-free linac improves treatment delivery efficiency in stereotactic body radiation therapy. *J Appl Clin Med Phys*, **14**(3): 64-71.
- Kry SF, Vassiliev ON, Mohan R (2010) Out-of-field photon dose following removal of the flattening filter from a medical accelerator. *Phys Med Biol*, **55**(8): 2155-2166.
- Spruijt KH, Dachele M, Cuijpers JP, et al. (2013) Flattening filter free vs flattened beams for breast irradiation. *Int J Radiat Oncol Biol Phys*, **85**(2): 506-513.
- Stieb S, Lang S, Linsenmeier C, et al. (2015) Safety of high-dose-rate stereotactic body radiotherapy. *Radiat Oncol*, **10**(27):1-8.
- Navarra P, Ascolese AM, Mancos P, et al. (2013) Volumetric modulated arc therapy with flattening filter free (FFF) beams for stereotactic body radiation therapy (SBRT) in patients with medically inoperable early stage non small cell lung cancer (NSCLC). *Radiother Oncol*, **107**(3): 414-418.
- Mancosu P, Castiglioni S, Reggiori G, et al. (2012) Stereotactic body radiation therapy for liver tumours using flattening filter free beam: dosimetric and technical considerations. *Radiat Oncol*, **7**(16): 1-8.
- Prendergast BM, Dobelbower MC, Bonner JA, et al. (2013) Stereotactic body radiation therapy (SBRT) for lung malignancies: preliminary toxicity results using a flattening filter-free linear accelerator operating at 2400 monitor units per minute. *Radiat Oncol*, **8**(273): 1-8.
- Prendergast BM, Popple RA, Clark GM, et al. (2011) Improved clinical efficiency in CNS stereotactic radiosurgery (SRS) using flattening filter free (FFF) linear accelerator. *53rd ASTRO Meeting* 3452.
- Wang Y, Khan MK, Ting JY, et al. (2012) Surface dose investigation of the flattening filter-free photon beams. *Int J Radiat Oncol Biol Phys*, **83**(2): 281-285.
- Mu X, Lofroth PO, Karlsson M, et al. (2003) The effect of fraction time in intensity modulated radiotherapy: theoretical and experimental evaluation of an optimization problem. *Radiother Oncol*, **68**(2): 181-187.
- Moiseenko V, Nanath JP, Duzenli C, et al. (2008) Effect of prolonging radiation delivery time on retention of gammaH2AX. *Radiat Oncol*, **3**(18).
- Lohse I, Lang S, Hrbacek J, et al. (2011) Effect of high dose per pulse flattening filter-free beams on cancer cell survival. *Radiother Oncol*, **101**(1): 226-232.
- Karan T, Moiseenko V, Gill B, et al. (2013) Radiobiological effects of altering dose rate in filter-free photon beams. *Phys Med Biol*, **58**(4): 1075-1082.
- Ito A, Nakano H, Kusano Y, et al. (2006) Contribution of indirect action to radiation-induced mammalian cell inactivation: Dependence on photon energy and heavy-ion LET. *Radiat. Res*, **165**: 703-712.
- Nunez MI, McMillan TJ, Valenzuela MT, et al. (1996) Relationship between DNA damage, rejoining and cell killing by radiation in mammalian cells. *Radiother Oncol*, **39**: 155-165.
- Rockwell S, Dobruck IT, Kim EY, et al. (2009) Hypoxia and radiation therapy: Past history, ongoing research, and future promise. *Curr Mol Med*, **9**(4): 442-458.
- Höckel M and Vaupel P (2001) Tumor hypoxia: Definitions and current clinical, biologic, and molecular aspects. *J Natl Cancer Inst*, **93**(4): 266-276.
- Hirayama R. (2014) Mechanism of Oxygen Effect for Photon and Heavy-ion Beams. *Jpn J Med Phys*, **34**(2): 65-69.
- Wozny AS, Alphonse G, Montagne PB, et al. (2016) Influence of Dose Rate on the Cellular Response to Low-and High-LET radiations. *Front Oncol*, **6**(58): 1-7.
- Bristow RG and Hill RP (2008) Hypoxia and metabolism: Hypoxia, DNA repair and genetic instability. *Nat Rev Cancer*, **8**: 180-192.
- Mathews LA, Cabarcas SM, Hurt E (2012) DNA Repair of Cancer Stem Cells. *Springer*, P115
- Rockwell S and Kallman RF (1973) Cellular Radiosensitivity and Tumor Radiation Response in the EMT6 Tumor Cell System. *Radiat Res*, **53**(2): 281-294.
- Setsukinai K, Urano Y, Kakinuma K, et al. (2003) Development of Novel Fluorescence Probes That Can Reliably Detect Reactive Oxygen Species and Distinguish Specific Species. *J Biol Chem*, **278**(5): 3170-3175.
- Meng A, Jalali F, Cuddihy A, et al. (2005) Hypoxia down-regulates DNA double strand break repair gene expression in prostate cancer cells. *Radiother Oncol*, **76**: 168-176.
- Kumareswaran R, Ludkovski O, Meng A, et al. (2011)

- Chronic hypoxia compromises repair of DNA double-strand breaks to drive genetic instability. *J Cell Sci*, **125**: 189-199.
34. Takagi K and Hatashita M (2006) Formation of Phosphorylated Histon 2AX Foci in the Mouse Fibroblast Cell Line. Report from Wakasa Energy Research Center, Fukui, Japan.
35. Kretschmer K, Sabatino M, Blehschmidt A, et al. (2013) The impact of flattening-filter-free beam technology on 3D conformal RT. *Radiat Oncol*, **8**(133).
36. Zhang W, Lin Z, Yang Z, et al. (2015) Evaluation of the dosimetric impact of applying flattening filter-free beams in intensity-modulated radiotherapy for early-stage upper thoracic carcinoma of oesophagus. *J Med Radiat Sci*, **62**(2): 108-113.

